

Integrated gas chromatograph

Jan A. Dziuban, Jerzy Mróz, and Jan Koszur

Abstract—A portable gas chromatograph with integrated micromachined flushed injector and thermal mass detector (TCD) has been developed. The silicon/glass injector operates in a fixed volume ($2 \times 7 \mu\text{L}$) or electronically operated mode. An integrated, pneumatically operated, fast cross-valve is applied in the injector. The TCD detector consists of two Pt microheaters and thermoresistors packaged in a silicon/glass micromachined chip. The temperature of two capillary molecular sieve separation columns is controlled by a thick-film heater fabricated on polyimide foil. The chromatograph is equipped with two 16-bits microprocessors communicating with the external portable PC. The instrument may operate in the on-line continuous analysis mode.

Keywords—portable gas chromatograph, integrated injectors, silicon micromechanics.

1. Introduction

In this paper the results of a long-lasting research program on portable gas chromatograph are presented. The program was carried out under the auspices of the State Committee for Scientific Research. The main goal of the research was to obtain a miniature gas chromatograph (GC) with a flushed gas injector and fast, nano-dead-volume TCD. The device is equipped with appropriate software and analog/digital circuits and is capable of ensuring continuous detection of combustible atmosphere in deep coal mining industry and/or continuous monitoring of the environment (long-term air quality, drifts, emission of pollutants, etc.).

2. Experiment

The portable gas chromatograph consists of two micromachined parts: a fixed or electronically adjusted gas injector and thermal-mass-detectors. Restek (USA) ID 0.32 mm Rt-Msieve 5A capillary columns, each 10 m long, are positioned in a thermally isolated chamber. A thick-film heater fabricated on elastic polyimide foil surrounds the columns and ensures proper adjustment and stabilization of the temperature ($50\text{--}120^\circ\text{C}$) (see Fig. 1).

The injector consists of two Borofloat 33 glass substrates, silicon (100) deep-micromachined substrate polished on both sides, and polyimide foil coated with Teflon®. The gas circuit of the injector includes one integrated fast cross-valve (1 ms) operated pneumatically, two fixed-volume chambers ($7 \mu\text{L}$ each) and two narrow channels for active and reference gas column supplying (Fig. 2). The fabrication process of the injector includes new processes of 3D-structure substrate-by-substrate assembling: selective bonding of glass and silicon substrate using polyimide foil (Fig. 3).

The TCD sensor applied in the GC has been designed and fabricated by the Institute of Electron Technology in Warsaw. In the device a thin-film Pt heater and a thermo-resistor

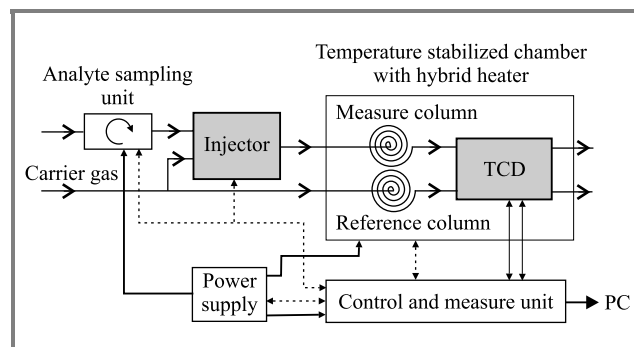


Fig. 1. Block diagram of the gas chromatograph with integrated micromachined components – gas injector and TCD sensor (grey areas).

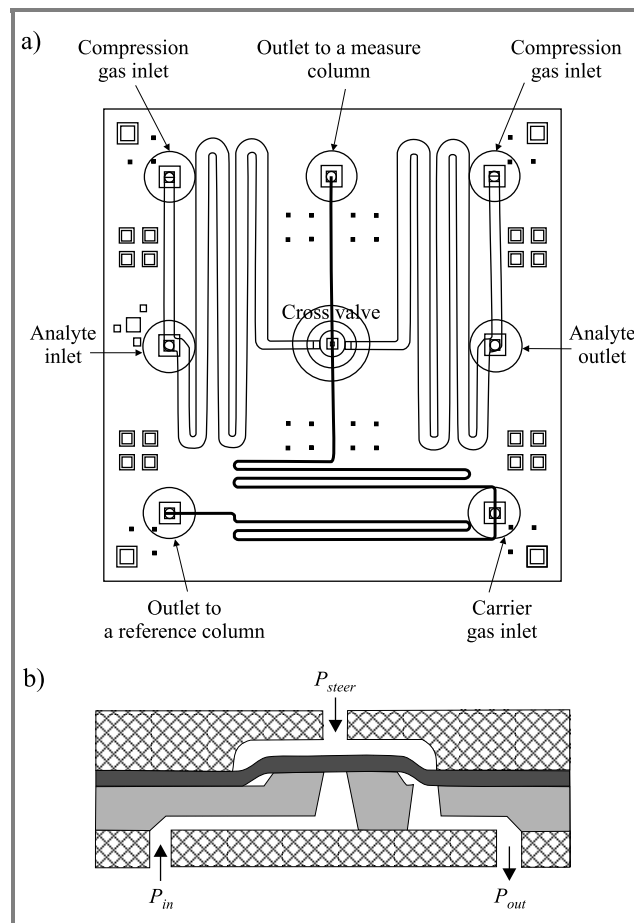


Fig. 2. The injector: (a) layout of the device; (b) cross-section of a microvalve; for $P_{steer} < P_{in}$ the microvalve is closed.

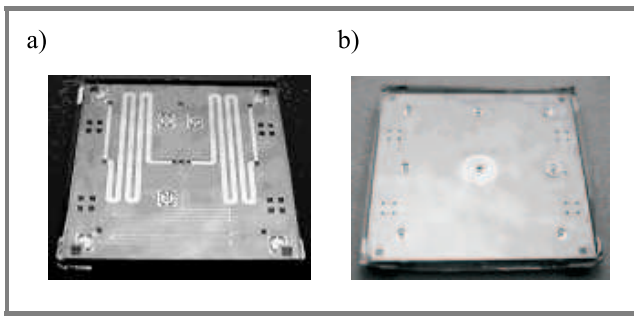


Fig. 3. The injector: (a) front-side: gas channels, fixed volume chambers and microvalve (in the middle) may be seen; (b) back-side view: analyte, carrier gas and control pressure inlets.

have been formed on a perforated membrane made of a double-layer SiO₂/Si₃N₄ system fabricated using LPCVD. The membrane extends over a gas channel formed by means of deep wet etching of a (100) silicon wafer. This structure is covered with a glue-bonded, 1 mm thick glass plate. The device chip is assembled with the capillaries and packaged in a metallic case, then wire-bonded connections are made (Fig. 4).

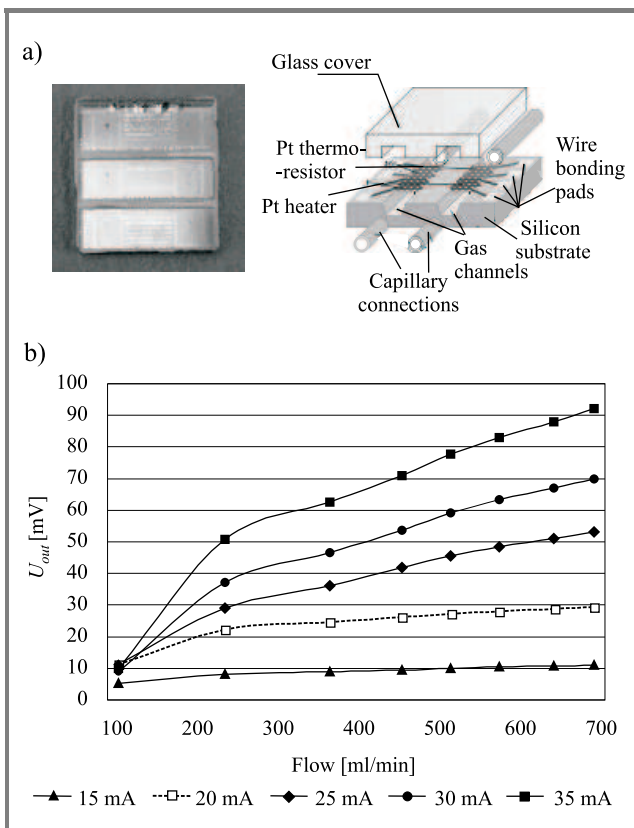


Fig. 4. TCD detector: (a) diagram (right) and view of the fabricated device (left); (b) most important characteristics – U_{out} versus N_2 flow for different levels of supply current.

In the solution reported here two independent sensors have been formed in a single chip and connected in the full Wheatstone bridge configuration in the self-calibrating mode.

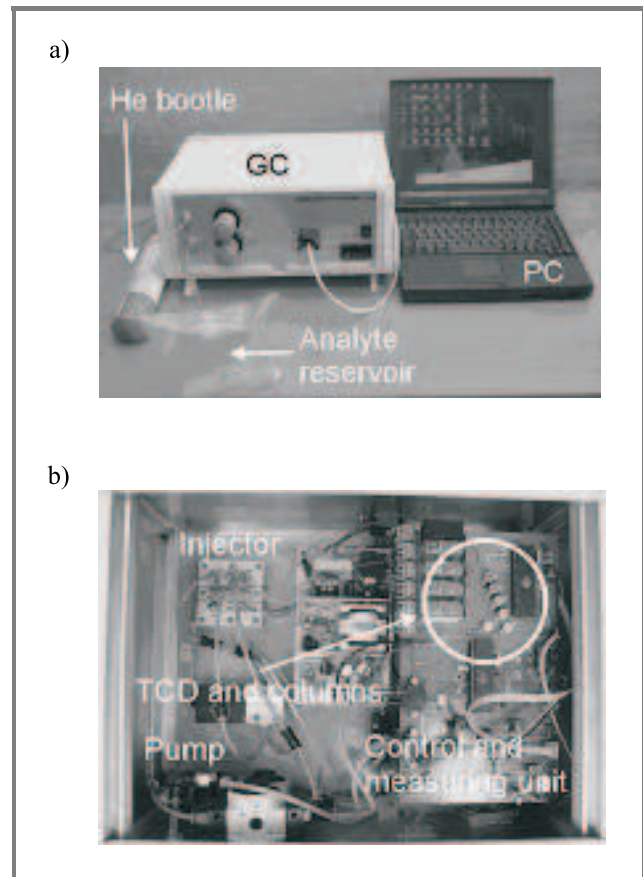


Fig. 5. Portable gas chromatograph: (a) the instrument, carrier gas bottle, and PC; (b) inside view.

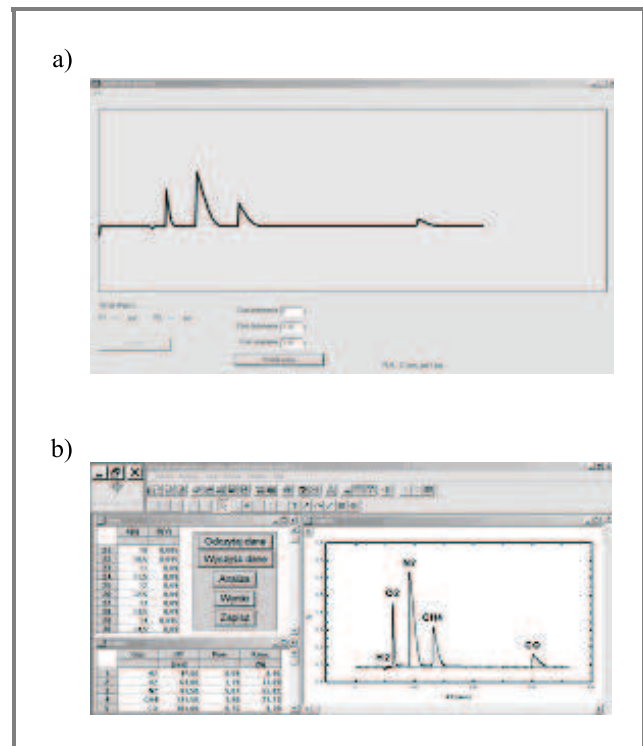


Fig. 6. Results of analysis: (a) electrical output signal and virtual control board of the GC; (b) processed chromatogram of a gas mixture and data table.

Table 1
Technical parameters of the GC reported here

<p>Dimensions/weight: 15 cm × 45 cm × 30 cm/~ 3.5 kg</p> <p>Environmental conditions: Indoor, automatic sampling from atmosphere (build in pump) or external source of analyte</p> <p>Supply: 230 V_(AC), 50–60 Hz, 200 VA</p> <p>Carrier gas: Helium carrier gas, external source, min. pressure 220 kPa</p> <p>Analysis time: Depends on gas mixture and applied column, 400–700 s</p> <p>Injector: Silicon/glass micromachined with polyimide membrane, the volume of injected analyte determined by cross-valve open time or total volume of the dosage loop (14 μL ± 1%), possible backflush and independent temperature stabilization</p> <p>Detector: Silicon/glass micromachined two-way thermo conductive detector (TCD) with four Pt micro spirals set up in auto compensating Whetstone's bridge circuit, death volume in nL range</p> <p>Chromatographic column: Depends on application (RT-Msieve 5 A, 10 m long, temperature 50–150°C)</p> <p>Control unit/software: External PC laptop-type with RS 232 or USB port, specialized software under Windows98/NT/2000/XP platform, all parameters of analysis electronically adjusted</p>

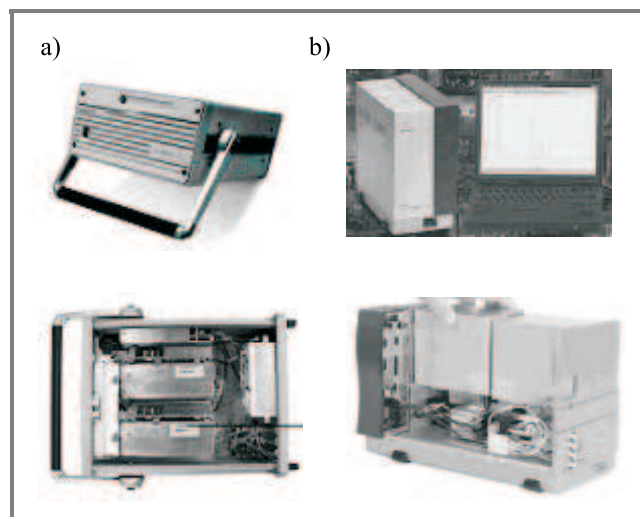


Fig. 7. The competing portable GCs: (a) Agilent 3000 Micro-GC; (b) Varian CP-4900 Micro-GC.

A printed circuit board with two 16-bit microcontrollers and specialized software designed and fabricated by the Institute of Automation and Electrification of Mining Industry – EMAG is used in the chromatograph.

The GC has been mounted in a metal box containing gas/electrical facilities (pump, pressure regulators and sensors, control valves). Both the injector and the TCD with the capillary columns enclosed in a thermally stabilized case are assembled in this box (Fig. 5).

The GC is able to operate either in the single-shot or in the continuous, automatic mode of analysis. All parameters of an analysis have to be set up by software from an external portable PC. The pressure of the carrier gas has to be adjusted manually, prior to the first analysis.

Chromatograms of gas mixtures may be observed immediately (real-time measurements), stored in memory and edited in the form table data and processed chromatograms with the description of detected gases added (Fig. 6).

Technical parameters our GC are similar to those of the well known Agilent/HP instrument (Table 1). The external view of both devices is shown in Fig. 7.

3. Conclusions

The most advantageous feature of our GC is the technical solution applied (possible only due to a complex know-how procedure). The approach resulted in technical parameters similar to those obtained by big producers of similar equipment in the world.

It is well known that the first integrated gas chromatograph was developed in the late 70's of the 20th century by Angell, Terry and Jerman [1]. After several years of redesigning, production of the portable gas chromatograph was undertaken by MTI Inc. (USA) and carried out in the late 80's and early 90's. Later the instrument became widely used under the name of Hewlett Packard (Agilent USA, <http://www.chem.agilent.com>).

At the moment, few projects devoted to the development of integrated gas chromatographs exist in Europe [2, 3], although many companies have been developing their own custom-designed gas meters based on the solutions used by Agilent. The lack of an independent market of key components and/or assembled portable gas chromatographs is the most important barrier blocking wider application of miniature gas chromatographs for on-line analysis in environment protection, gas systems electroengineering systems, etc.

We have built a portable (weighting approx. 3.5 kg) gas chromatograph for continuous analysis of a gas mixture. The lowest detection level obtained is a few ppm, the average analysis time is below 6 minutes (depending on a column applied), the repetition time is 10 seconds. All parameters of the GC may be adjusted electronically, the results of the analysis may be visualized immediately. At the moment it seems that our gas chromatograph is the only European solution comparable to Agilent/HP standards.

We would like to emphasize that the GC presented here is the effect of a long-lasting cooperation between several partners from academic and research institutes in Poland (Wrocław, Warsaw, Katowice). The success of this shared effort relies heavily on programs of the State Committee for Scientific Research PBZ 2705 (basic technologies

applicable in GC fabrication) and PBZ 01915, as well as on other projects carried out by EMAG Katowice.

We hope that good scientific results reported here will be followed by technology transfer and industrial implementation of the integrated GC.

Acknowledgements

We would like to thank the graduate students of the Faculty of Electronics and Faculty of Microsystems Electronics and Photonics of Wrocław University of Technology Wojciech Bula and Dawid Zalewski for their help, to Dr. Rafał Walczak, Dr. Anna Górecka-Drzazga, Dr. Łukasz Nieradko, Dr. Krzysztof Małecki of Faculty of Microsystems Electronics and Photonics of the above mentioned University, and Dr. Małgorzata Szczygielska and Marcin Małachowski of the Center EMAG Katowice for the development and fabrication of the integrated components and GC. Last but not least, we would like to express our deepest appreciation of the technological effort of Paweł Kowalski, Dr. Jan Łysko, Jerzy Jaźwiński and Dr. Zenon Gniazdowski of the Institute of Electron Technology from Warsaw.

The research has been financed (mainly) by PBZ 01915 and (partly) 9T11A03710 programs of the State Committee for Scientific Research.

References

- [1] S. Terry, J. Jerman, and J. Angell, "A gas chromatographic air analyzer fabricated on silicon wafer", *IEEE Trans. Electron. Dev.*, vol. ED26, no. 2, pp. 1880–1886, 1979.
- [2] M. B. Stone and J. A. de Mello, "Life, the universe and microfluidics", *Lab Chip*, no. 2, pp. 58–64, 2002.
- [3] Actaris Inc., "The meter of natural gas" (unpublished technical letter).



Jan A. Dziuban was born in Sanok, Poland, in 1951. He got the M.Sc. degree in 1974, then Ph.D. in 1978 and D.Sc. in 2002. He has been Assistant Professor at Wrocław University of Technology since 1978, the Directeur de Recherche at CNRS Besancon, Institute FEMTO since 2004. He has been a member of the Board

of Polish Society of Sensor Technology since 1992, a member of Steering Committee of Eurosensors Con-

ference since 1993, a member of Steering Committee of IVNC since 1999, a member of Commission of Micro-engineering of PAS, Committee of Machines Building Polish Academy of Sciences since 2003. He is a founder of micromechanics of silicon in Poland. He is the author of over 110 scientific works and patents.

e-mail: Jan.Dziuban@pwr.wroc.pl

Faculty of Microsystem Electronics and Photonics

Wrocław University of Technology

Janiszewskiego st 11/17

50-372 Wrocław, Poland



Jerzy Mróz received the M.Sc. degree from the Mining Electrical Engineering Department, AGH University of Science and Technology in 1969 and Ph.D. degree in engineering in 1989. As an engineer, he worked in GIG on sensors of ventilation parameters in mines. Since 1975 he's been working in the Research and Develop-

ment Center for Electrical Engineering and Automation in Mining (EMAG). At present he is involved in the Safety Systems and Ventilation Control Department.

e-mail: mroz@emag.katowice.pl

The Research and Development Center

for Electrical Engineering and Automation

in Mining (EMAG)

Leopolda st 31

40-189 Katowice, Poland



Jan Koszur was born in Warsaw, Poland, in 1943. He received the M.Sc. degree from Department of Electronics, Warsaw University of Technology, Poland, in 1968. His scientific interest is focused on design and fabrication of the silicon microsystems. He is working now as a Chief of Silicon Sensors Department of

Institute of Electron Technology (IET), Warsaw.

e-mail: koszur@ite.waw.pl

Institute of Electron Technology

Lotników av. 32/46

02-668 Warsaw, Poland